


Unsafe Injection Practices and Disease Transmission

Reuse of syringes combined with the use of single-dose vials for multiple patients undergoing anesthesia can transmit infectious diseases. The syringe does not have to be used on multiple patients for this to occur.

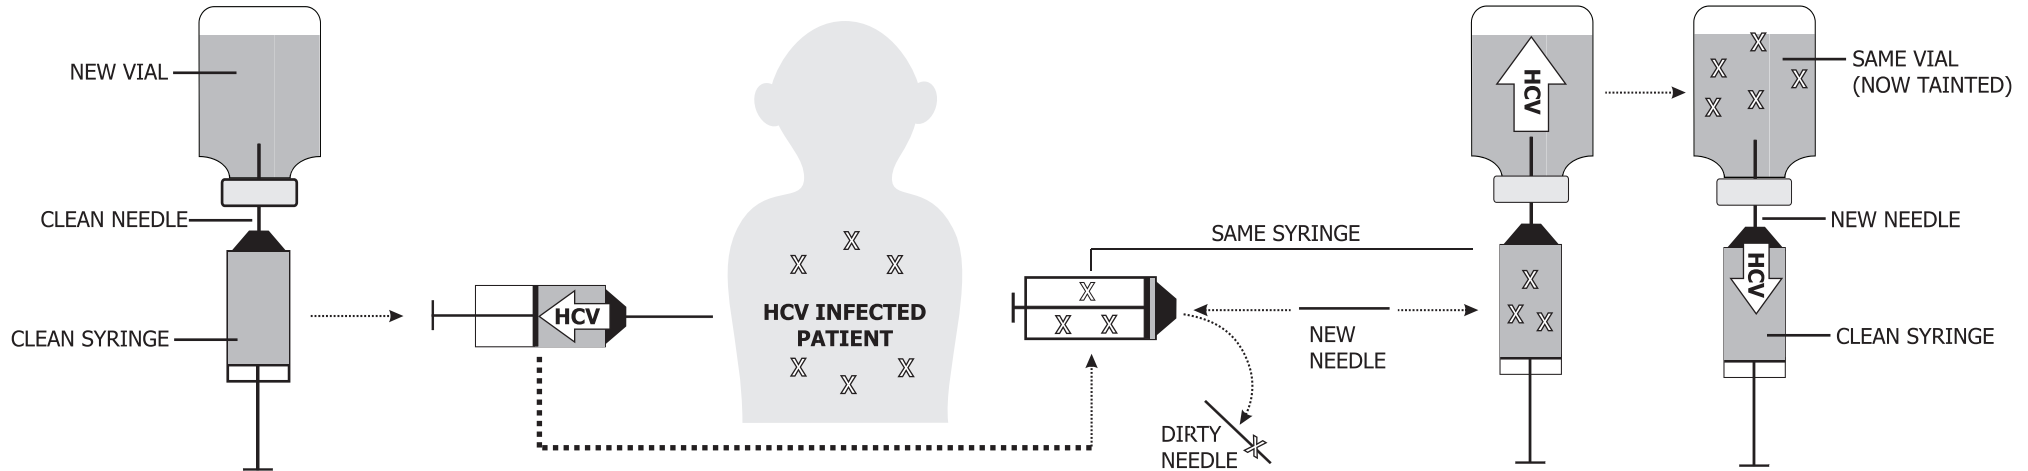

1. A clean syringe and needle are used to draw the sedative from a new vial.

2. It is then administered to a patient who has been previously infected with hepatitis C virus (HCV). Backflow into the syringe contaminates the syringe with HCV.

3. The needle is replaced, but the syringe is reused to draw additional sedative from the same vial for the same patient, contaminating the vial with HCV.

4. A clean needle and syringe are used for a second patient, but the contaminated vial is reused. Subsequent patients are now at risk for infection.